

FIG. 1

09993407-11501

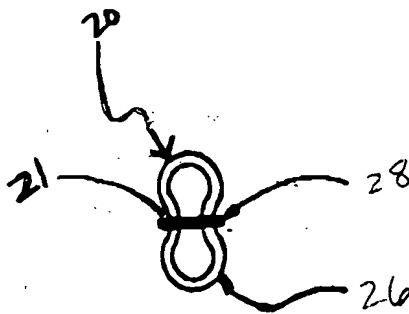


FIG. 2

09991407, 11501

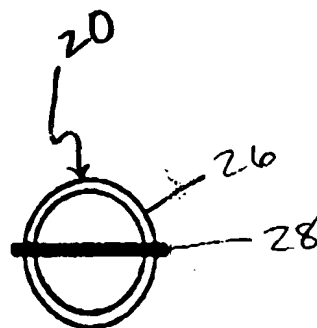


Fig. 3

0991407, 11501
FO977, 2047660

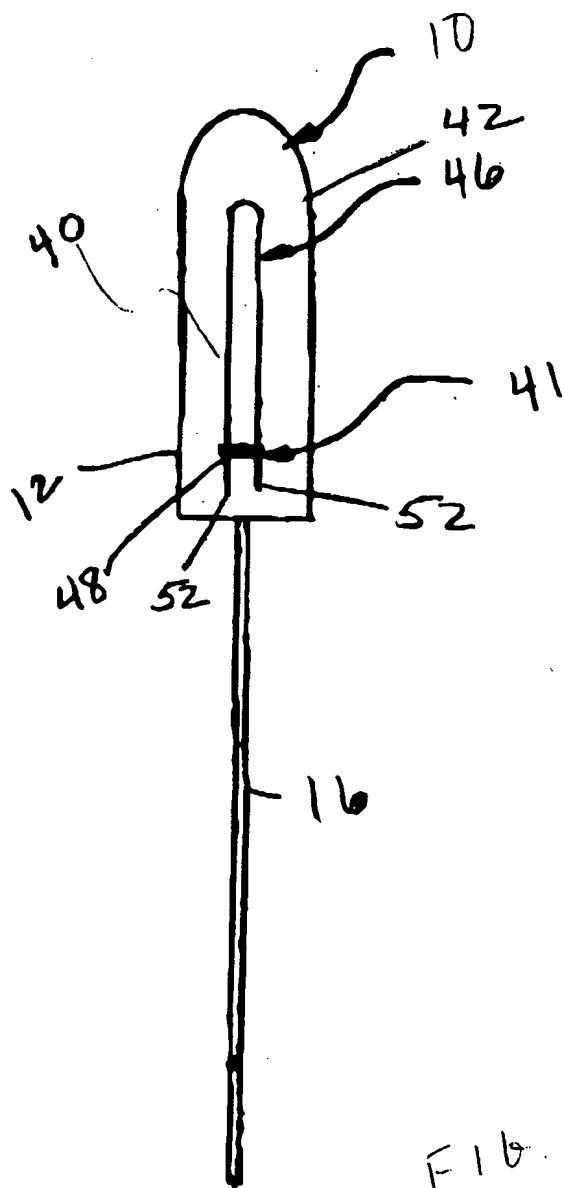


FIG. 4

09951407, 11501

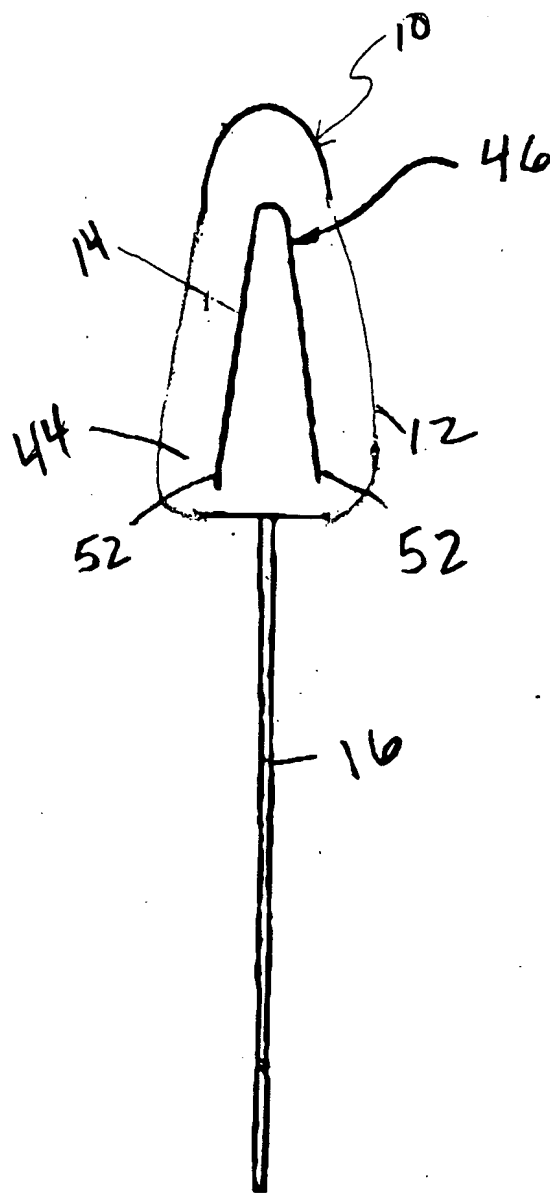


Fig. 5

09991407.111501

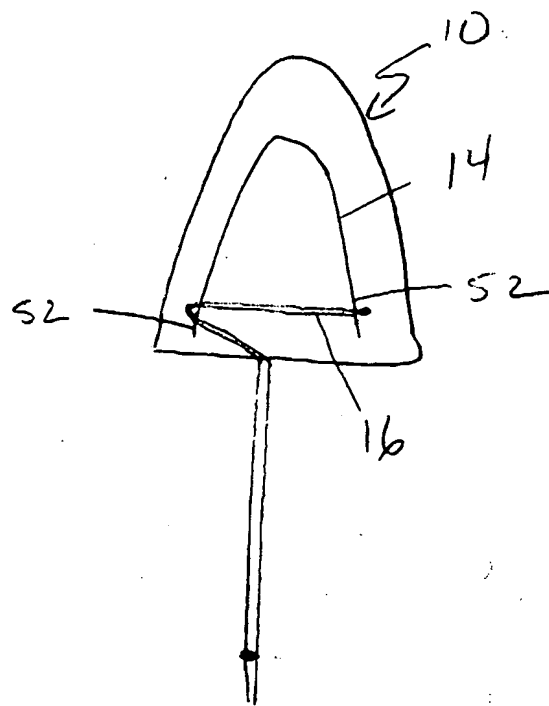


Fig. 5a

0991407 11501

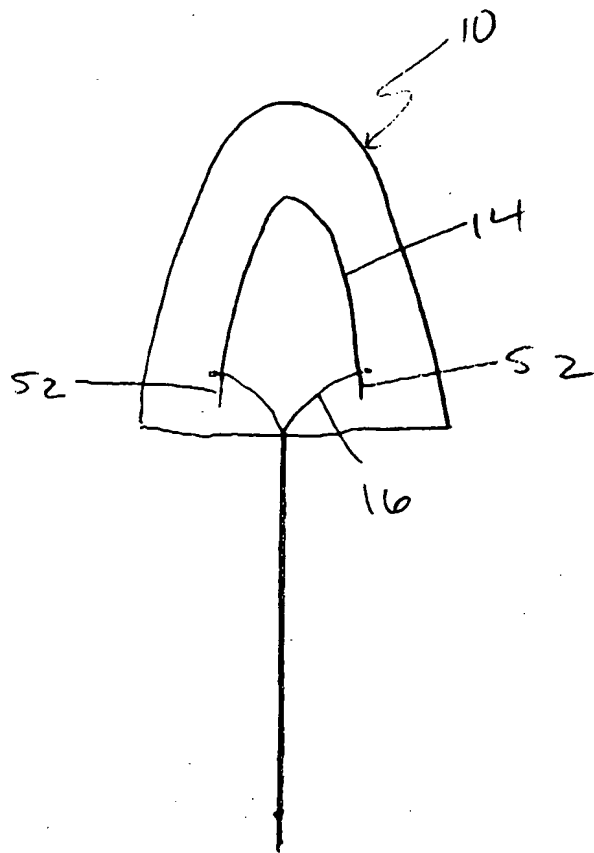


FIG. 5b

09991407 111601

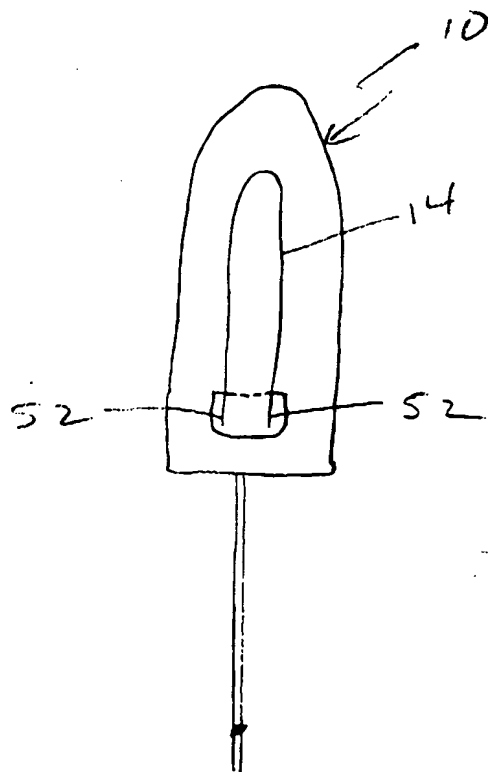


FIG. 5 C

0591403-11504

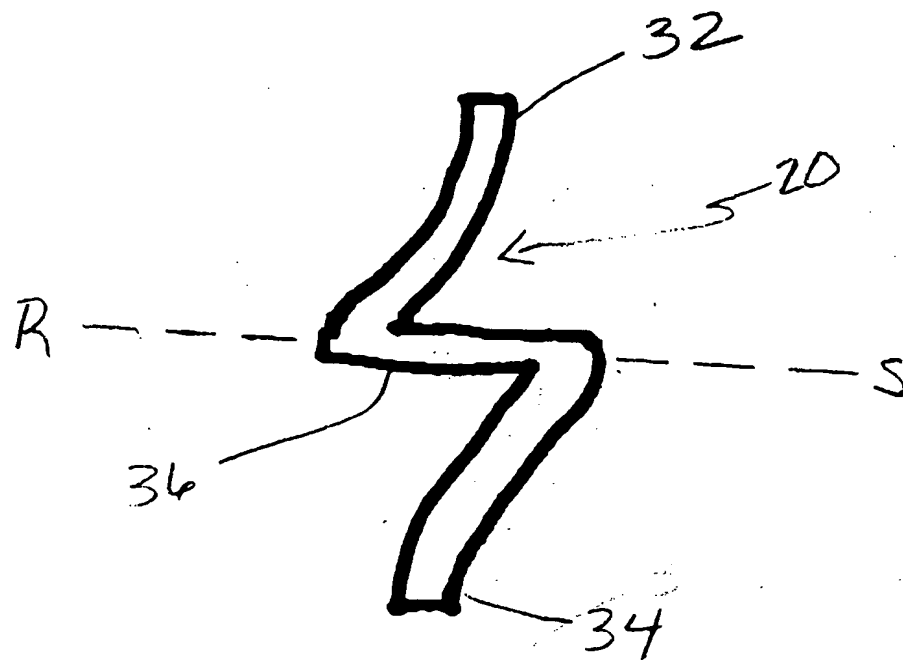


FIG. 6

00001407, 11501

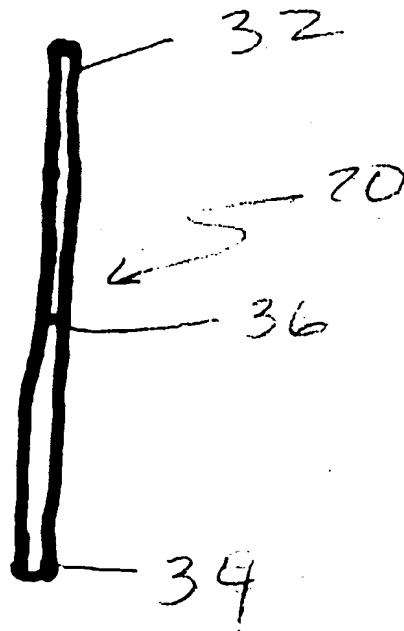


FIG. 7

34

09931402, 11501

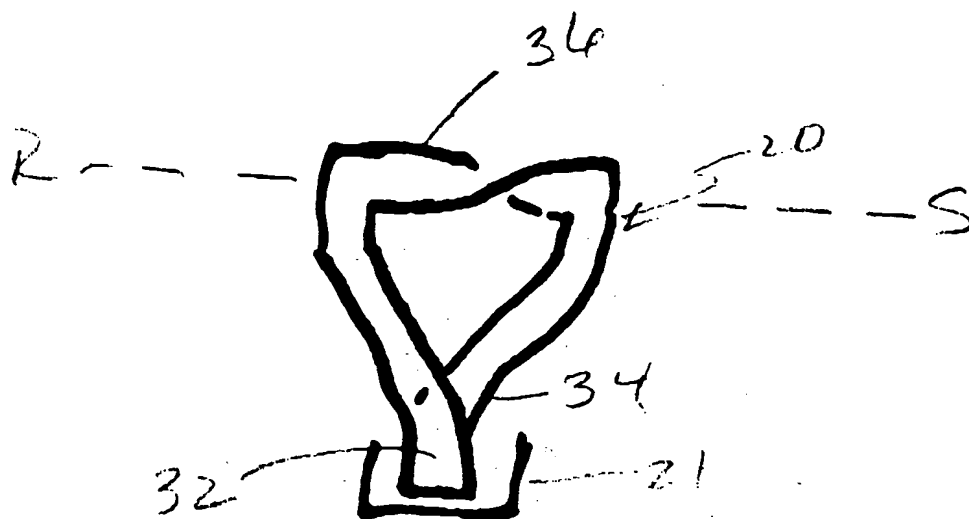


FIG. 8

09991407.111501

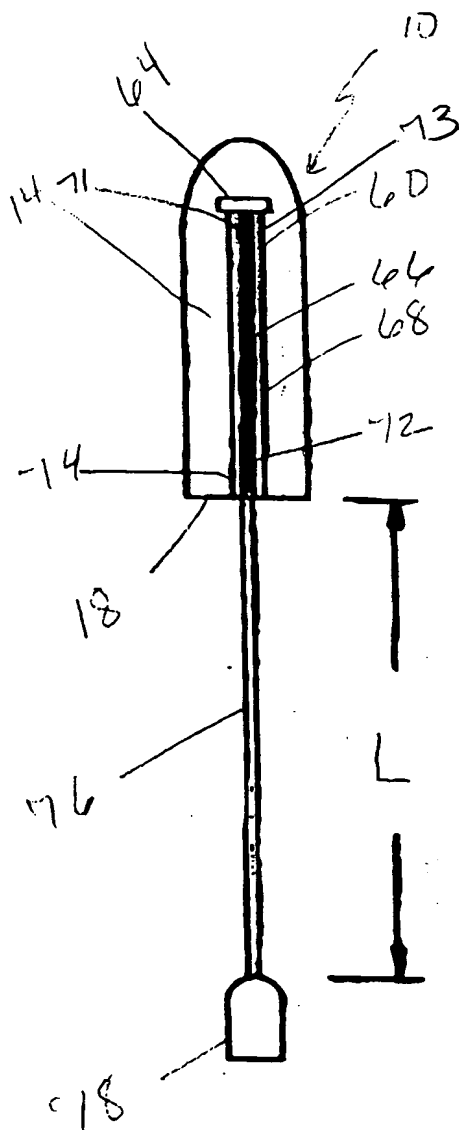


FIG. 9

09991487, 111501

"Catamenial Device Change Indicator"
Anthony DiSalvo, et al.
Docket No. PPC-812

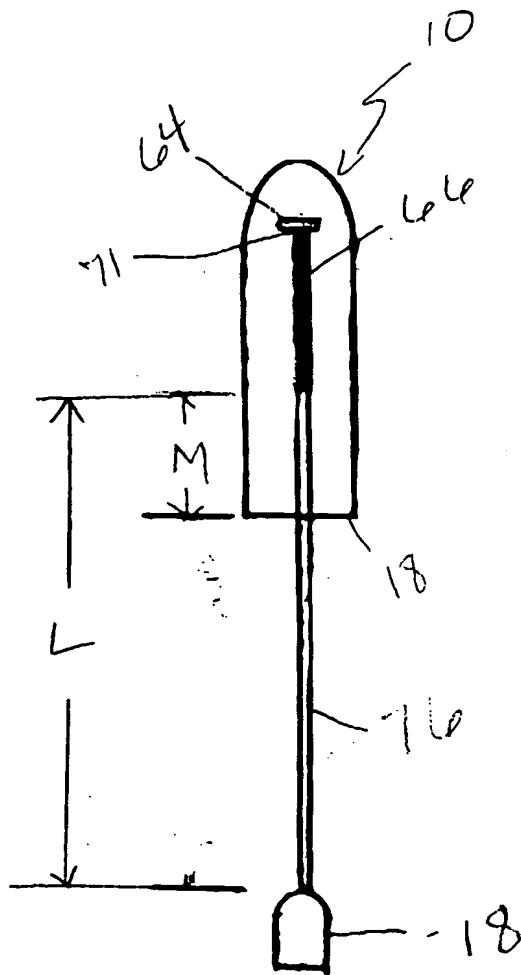


FIG. 16. 10

0991407, 11501

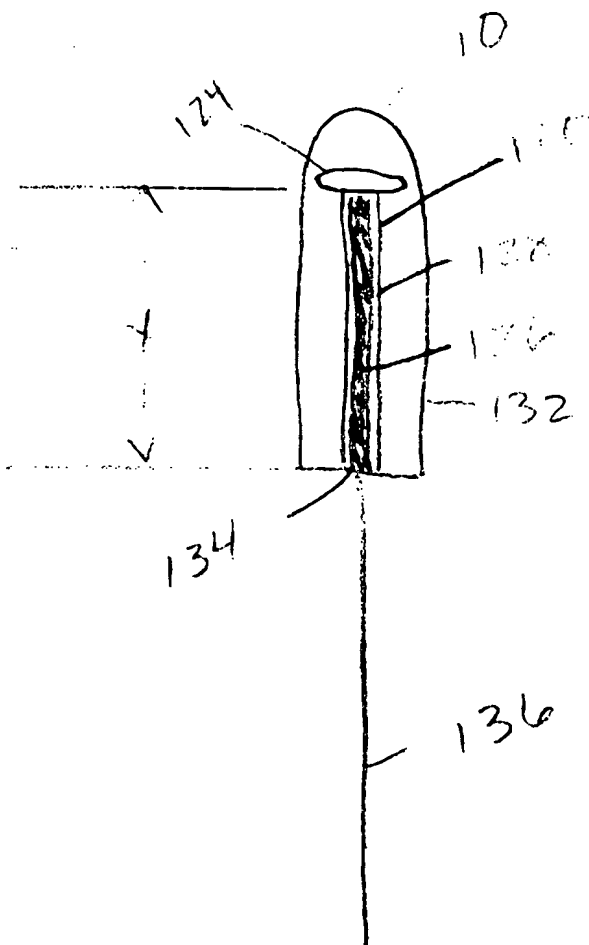


Fig. 11

0991402.11501

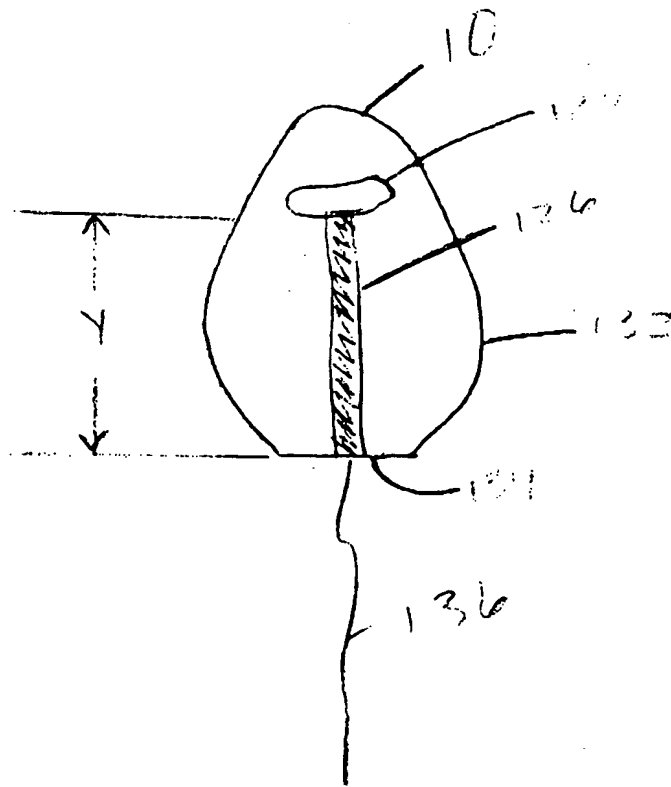


Fig. 12

0993407, 11501

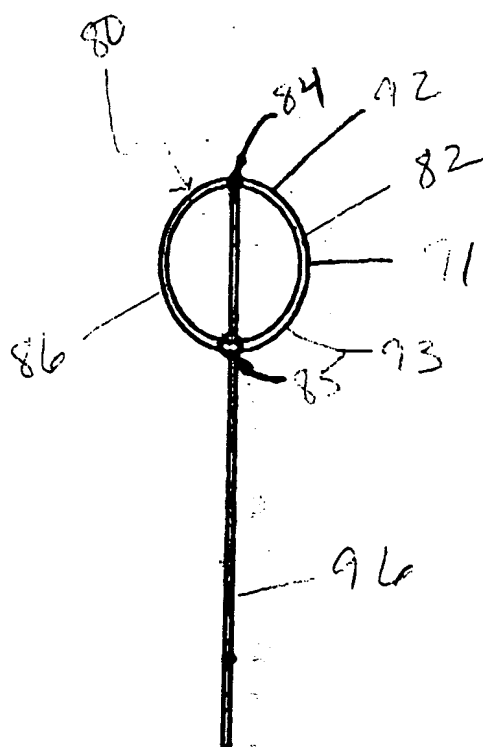


FIG. 13

0993407.11601

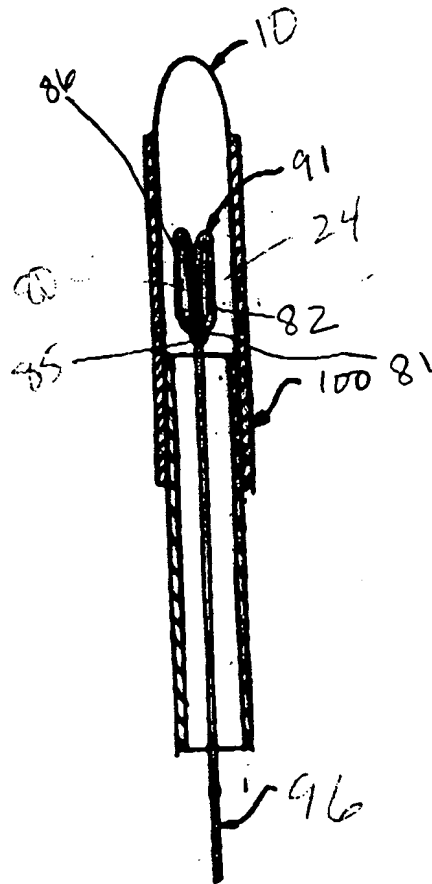


FIG. 14

0991407, 11501

09994407, 111501

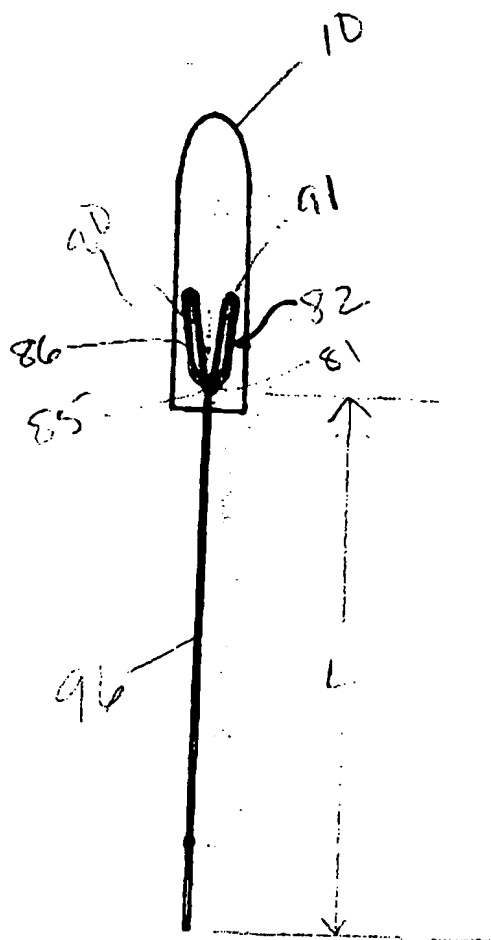


FIG. 15

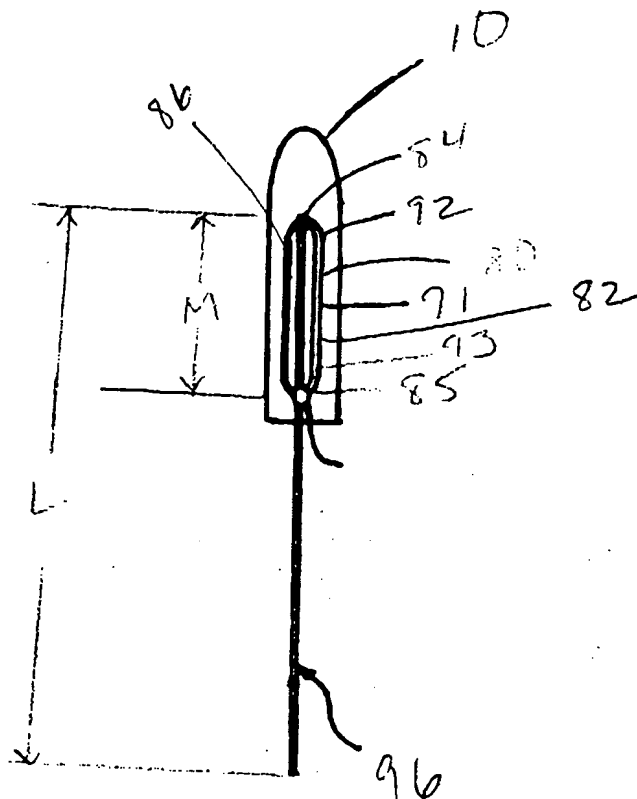


Fig. 16

00991407-11501

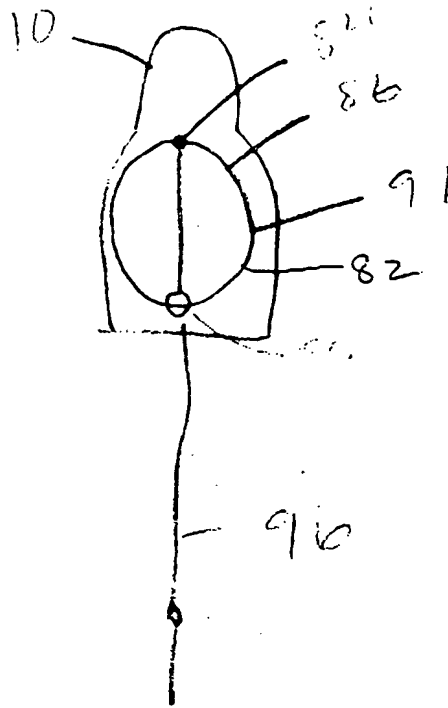


FIG. 17

09991407, 11501
FOSTER, 20476660